


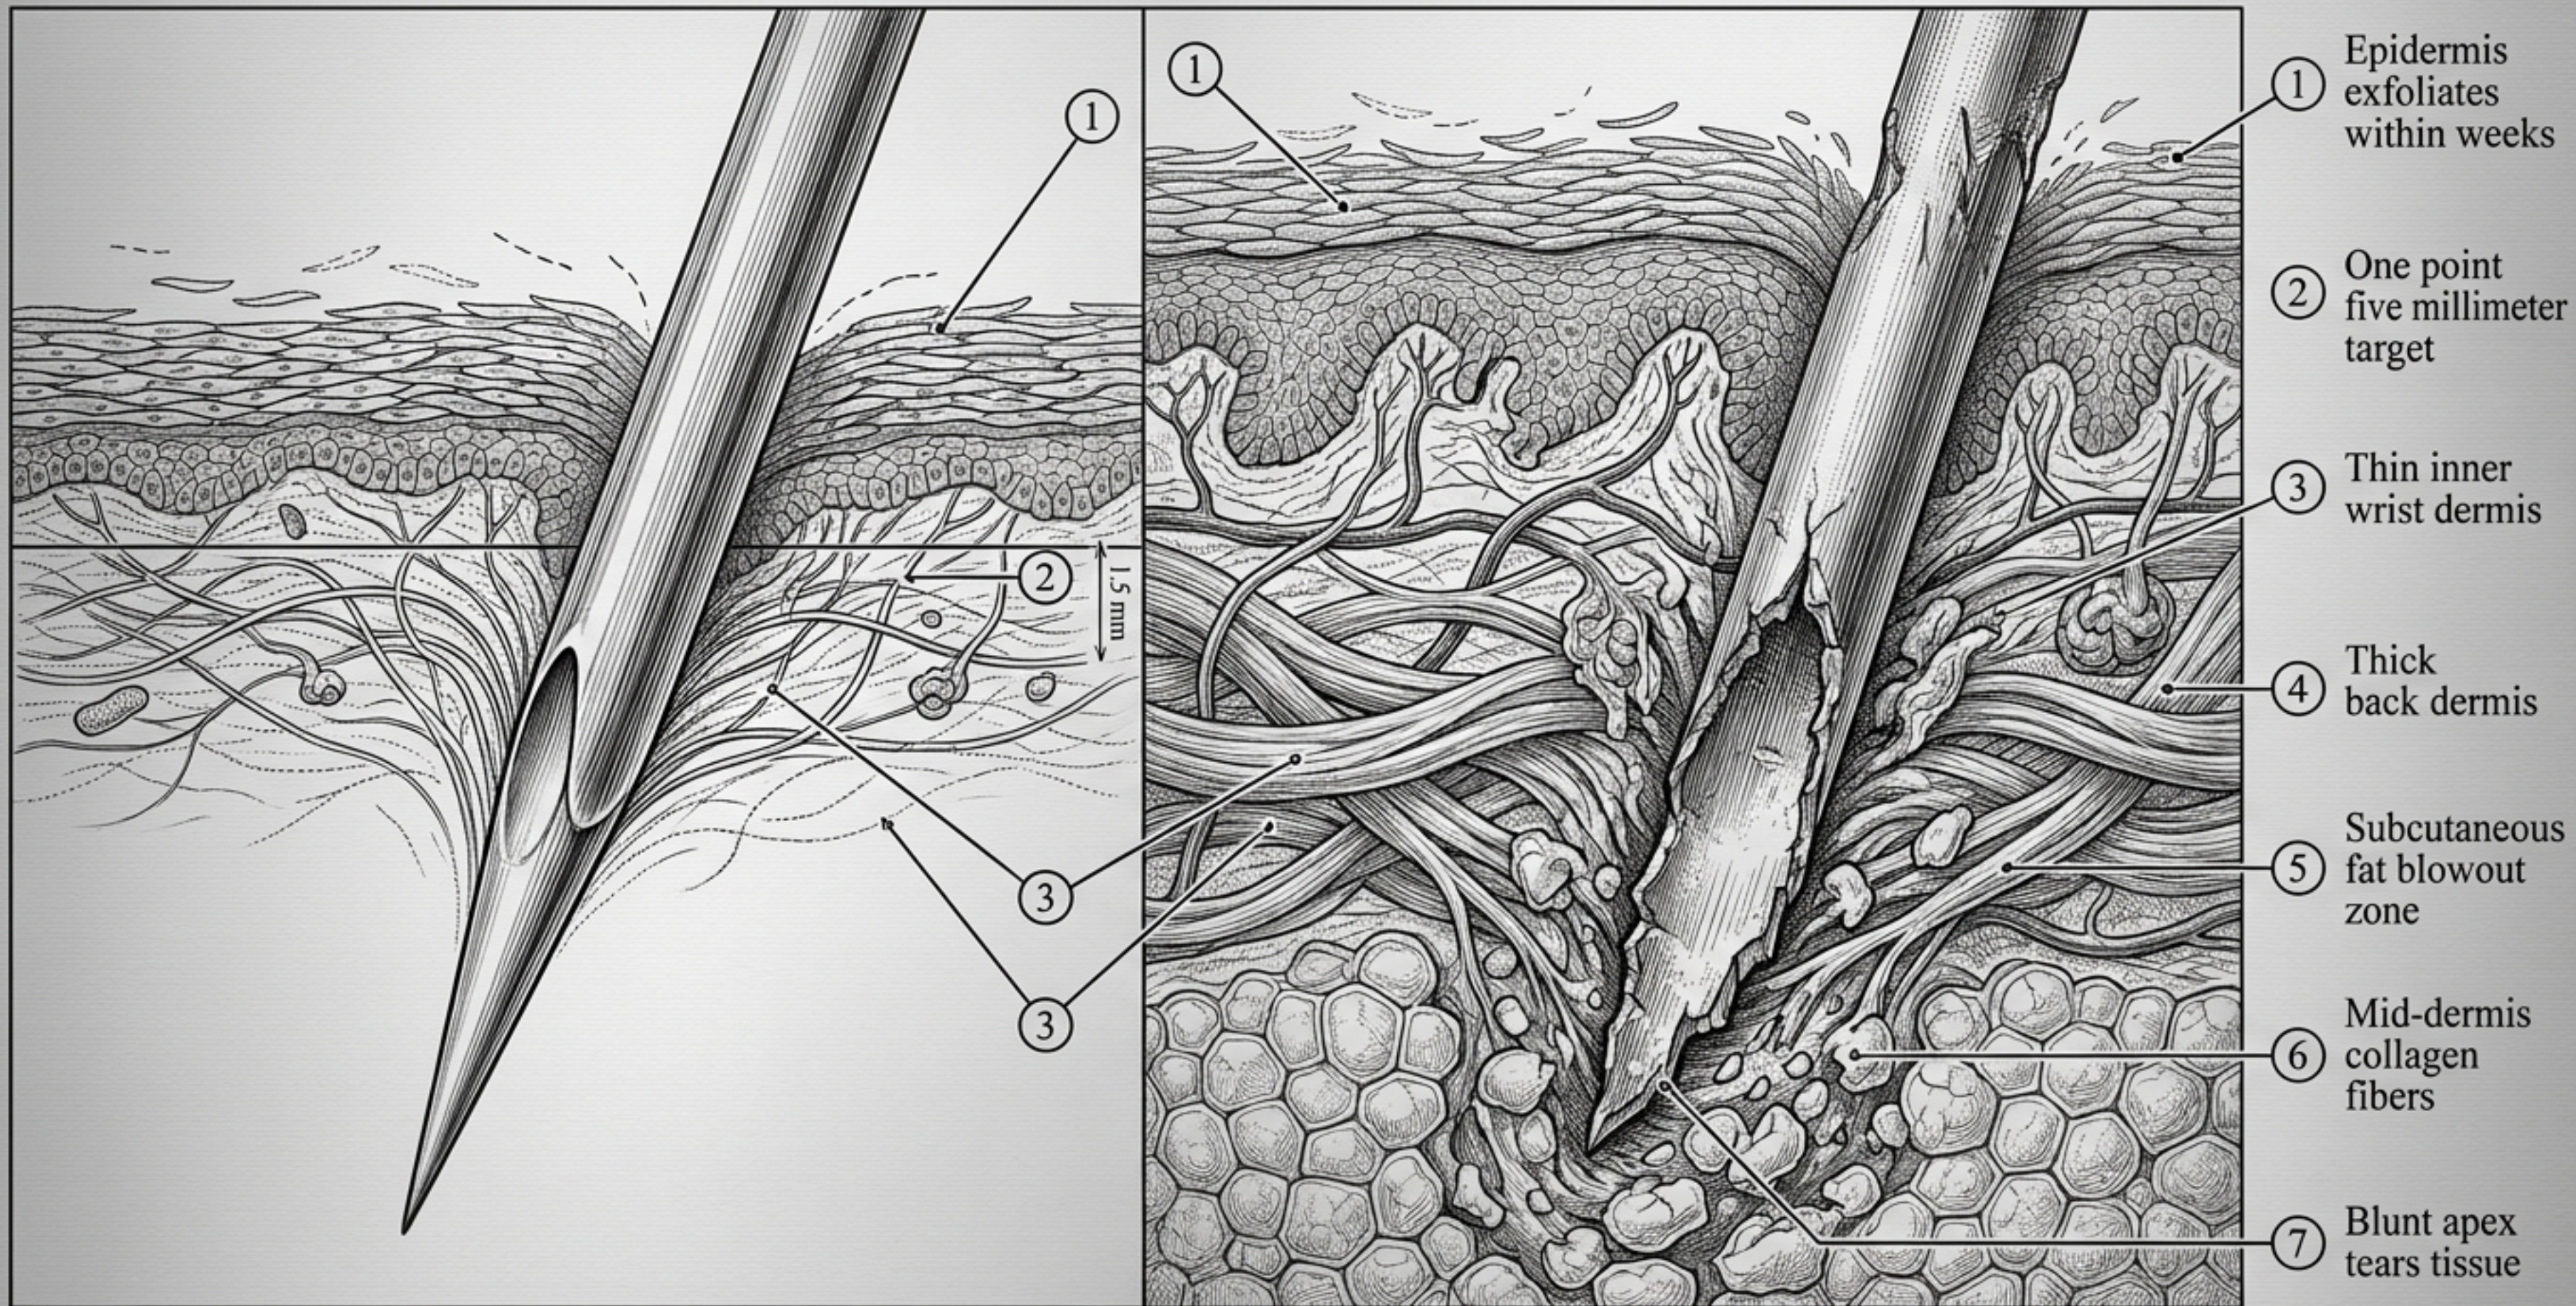

Skin thickness varies drastically by anatomical location, dictating strict needle depth calibration to avoid lateral diffusion.

STRATIFICATION AND DEPTH VARIANCES